



The antimicrobial effects of Cold Atmospheric Plasma jet on microorganisms causing dental caries (in vitro study)

Ghada Abdul Salam Ibrahim¹, Maha Jamal Abbas², and Eaman Ali AL-Rubae³

¹ Pedodontic and Preventive dentistry department, College of Dentistry, University of Baghdad/ Baghdad, Iraq

² Preventive Dentistry, College of Dentistry, Mustansiriyah University/ Baghdad, Iraq

³ Department of Basic Science, College of Dentistry, University of Baghdad/ Baghdad, Iraq

Correspondence: Ghada Abdul Salam Ibrahim

Email: ghadaalbaghdadi15@gmail.com

Received: 3 February 2023; Accepted: 28 April 2023; Published: 28 June 2023

Abstract

Aim of the study: The common microorganism in caries process are *Streptococcus mutans* and *Lactobacilli*. *Candida albicans* have correlation with *Streptococcus mutans* for enhanced dental caries. Cold Atmospheric Plasma (CAP) is called as non-thermal as result of electrons are more heated than heavy particles which are at room climate. CAP jets are ionized native gas outflow, produced underneath typical pressure through microwaves, high frequency or pulsed direct current employing noble gases. There are many applications of CAP in dentistry: in periodontology, implantology, prosthodontic, operative dentistry and in cariology. This study aimed to measure the sensitivity of the *S. mutans* and *C. albicans* to CAP jet.

Material and method: In this experiment, newly developed Cold atmospheric plasma jet (Iraqi made) using argon gas at a Gas flow rate 10 l/min, 175voltage and Frequency 2.45 GHz at room temperature such that the nozzle tip had a maximum distance of 2mm from the agar plate. Cold atmospheric plasma effect was tested at different times on the viable numbers of *Streptococci mutans* and *Candida albicans*.

Results: Through the irradiation of CAP jet on agar plates the antimicrobial efficacy for *S. mutans* and *C. albicans* was measured at different time the 3, 6, 9 minutes. Multiple pairwise comparisons using Tukey HSD showed there is significant reduction of colony forming unit (CFU) for *Streptococci mutans* by plasma at all time compared to control. Multiple pairwise comparisons using Tukey HSD showed there is highly significance differences for *C. albicans* was observed for all times in comparison to control ($p < 0.01$). The data of the current study was analyzed using statistical package for social science (SPSS version 22). Thus, it can be concluded that Cold Atmospheric plasma (argon gas) jet has anti-microbial efficacy against *Streptococci mutans* and *Candida albicans*. but it effects on *Candida albicans* more than on *Streptococci mutans*.

Keywords: Antimicrobial effects, Cold Atmospheric Plasma, *Streptococci mutans*, *Candida albicans*.

Introduction

The common microorganism in caries process are *Streptococcus mutans* and *Lactobacilli* ⁽¹⁾. *Streptococcus mutans* adhere to the enamel pellicle and to other plaque micorganism. They are acidogenic and acidouric creating the risk for dental caries ^(2,3). *C.albicans* act as an opportunistic

pathogen under certain condition cause a variety of infections, for instance, thrushes in infant and chronic atrophic candidiasis (denture -induced stomatitis) in adult ^(4, 5, 6, 7). *Candida albicans* have correlation with *Streptococcus mutans* for enhanced dental caries and severe oropharyngeal diseases ^(8, 9). Studies have confirmed a positive relation



between *Candida albicans* and initiation of dental caries in young adults and children^(10, 11, 12).

Plasma is most common form of matter (4th class of material). The British physicist Sir William Crookes explored Plasma in 1879, but the Irving Langmuir, an American chemist was determined name “plasma”, in the year 1929. Plasma is a group of stripped particles. Formerly the electrons are deprived from molecules and atoms, those particles modify situation and change to plasma⁽¹³⁾.

Classification of plasmas are classified as “thermal” or “non-thermal” according to temperatures of the ions, electrons, and neutrals⁽¹⁴⁾. Cold Atmospheric Plasma (CAP) is called non-thermal because it has electrons are more heated than heavy particles which are at room climate⁽¹⁵⁾. In last years, cold atmospheric plasma sources (below 40 °C) have been produced to expand plasma treatment to living cell⁽¹⁴⁾. Various methods to produce plasma include plasma needle, Atmospheric Pressure Plasma Jet (APPJ), plasma pencil and Dielectric Barrier Discharge (DBD). Gases be employed to generate CAP are Nitrogen, Argon, Helium, air and Heliox (a mix of helium and oxygen)⁽¹⁵⁾. CAP jets are ionized native gas outflows, produced underneath typical pressure through microwaves, high frequency or

pulsed direct current in so-named plasma-jet sources employing noble gases⁽¹⁶⁾.

There are many applications of CAP in dentistry: in periodontology, implantology, prosthodontic, operative dentistry and in cariology as antimicrobial therapeutic interventions against microorganisms causing dental caries. The antimicrobial effects are depended on the production of reactive oxygen (ROS) and nitrogen species (RNS) involving charged particles, free radicals, electric fields, and electric radiation such as Ultraviolet radiation^(17, 18, 19, 20, 21).

Goree et al, 2006⁽²²⁾ confirmed that CAP killed *Streptococcus mutans*, a gram-positive cariogenic bacterium. Subsequently, Yang et al. was found that CAP argon plasma brush was very efficient in killing *S. mutans* and *L. acidophilus*⁽²³⁾. CAP showed antifungal effect on *C. albicans* virulence factors, such as filamentation and adhesion⁽²⁴⁾.

CAP can irradiate and treat irregular surfaces; making them good for sterilization tooth cavity without need for preparation of tooth. CAP itself is superficial, but the active plasma species it give can freely enter inner the cavities⁽²⁵⁾. The aim of this study was to assess the sensitivity of the *S. mutans* and *C. albicans* to Cold Atmospheric Plasma (CAP) jet.

Material and methods

The Sensitivities of the *Streptococcus mutans* and *Candida albicans* to Cold atmospheric plasma:

In this experiment, newly developed Cold atmospheric plasma jet (Iraqi made) using argon gas at a Gas flow rate 10 l/min, 175volt and Frequency 2.45 GHz At room temperature such that the nozzle tip had a maximum distance of 2mm from the agar plate. This device was made in Baghdad University, College of Science for Girls, Department of Physics- Medical Physics laboratory for Postgraduate Studies. In this experiment, Cold atmospheric plasma effect was tested at different times (3, 6, 9) minutes on the viable numbers of *Streptococci mutans* and *Candida albicans*. Pure isolates of the bacteria and *Candida*, they were preserved in nutrient agar in the refrigerator until required for the study. Pure isolates of *Streptococcus mutans* and *Candida albicans* can be activated by addition 0.1 ml added to 10 ml of sterilized brain heart infusion broth, then incubated aerobically for 18 hr at 37 °C before each experiment ⁽²⁶⁾.

In these experiments 4 groups for *Streptococcus mutans* and *Candida albicans* (one control and others study groups). Standardized suspensions of bacterial and fungal broth that contained 1.5×10^8 colony forming units (McFarland Standard 0.5) were prepared. After plating 2 ml of each microbial broth onto the agar, the surface was aired slightly. The apex of the cylinder of CAP jet was placed at 90 angles to the surface of the agar plate and then CAP jet was placed at a length of 2mm from the agar plate. Plasma exposure times were 3, 6, 9 minutes respectively and compared with control before plasma exposure After plasma irradiation, bacteria and *Candida* was cultured on agar plates. Mitis-Salivarius Bacitracin Agar (MSB Agar), This media for culturing of *Mutans streptococci*. Sabouraud Dextrose Agar (SDA), This selective media

for culturing and isolation of *Candida albicans* and then measurements was decided by counting the living cells after plasma exposure by colony forming unit (CFU) and compared with control before plasma irradiation ⁽²⁷⁾.

CFU/ml = No. of colonies x 1/dilution factor x 10

Statistical analysis

Statistical Package for Social Research was used for descriptive analysis, and presentation (SPSS version -22, Chicago, Illionis, USA). Levene test for such a quantitative variable that includes the minimum, maximum, mean, standard deviation (SD), and standard error. Using Tukey's Honestly Significant Difference (Tukey's HSD) for multiple pairwise comparisons among group. Not significant with a P value more than 0.05, significant at a P value lower than 0.05.

Result

Through irradiation of CAP plasma jet on agar plates, the antimicrobial efficacy for *S. mutans* was measured at different time (3, 6, 9) minutes as shown in figure and table 1 . Multiple pairwise comparisons using Tukey HSD showed there is significant reduction of colony forming unit (CFU) for *Streptococci mutans* by plasma at all time compared to control as shown in table 2. When compared between treatment group there is significant reduction of colony forming unit($p < 0.05$). the antimicrobial effect of *C. albicans* was measured at different time (3, 6, 9) minutes as shown in figure 2 and table 3. Multiple pairwise comparisons using Tukey HSD showed there is highly significance differences was observed for all times in comparison to control before irradiation of plasma ($p < 0.01$). When compared between treatment group there is no significant

reduction of colony forming unit ($p < 0.05$)
(table 4).




Figure 1: Sensitivities of *Streptococcus mutans* exposed to plasma at different exposure times (A) control (B) After 3 minutes (C) After 6 minutes (D) After 9 minutes




Figure 2: Sensitivities of *Candida albicans* exposed to plasma at different exposure times (A) control (B) After 3 minutes (c) After 6 minutes (D) After 9 minutes

Table 1: Descriptive and statistical test of colony forming unit (CFU) for *Streptococci mutans* exposed to plasma

Statistics	Control	3 mins.	6 mins.	9 mins.	F	P value
Minimum	250.000	100.000	80.000	175.000	41.050	0.000
Maximum	300.000	270.000	225.000	298.000		
Mean	287.700	174.400	156.100	228.200		
±SD	17.783	63.483	52.069	55.226		
±SE	5.623	20.075	16.466	17.464		

Table 2: Multiple pairwise comparisons of colony forming unit (CFU) for *Streptococci mutans* exposed to plasma using Tukey HSD

(I) time	(J) time	Mean Difference (I-J)	p value
Baseline	3 mins.	113.300	0.001
	6 mins.	131.600	0.000
	9 mins.	59.500	0.046
2	6 mins.	18.300	0.039
	9 mins.	-53.800	0.001
3	9 mins.	-72.100-	0.000




Figure 3: Sensitivities of *Streptococcus mutans* exposed to plasma at different exposure times (A) Control (B) After 3 minutes (C) After 6 minutes (D) After 9 minutes

Table 3: Descriptive and statistical test of colony forming unit (CFU) for *Candida albicans* exposed to plasma

Statistics	Control	3 min	6 min.	9 min.	F	P value
Minimum	50.000	2.000	1.000	1.000	29.702	0.0000 Sig.
Maximum	125.000	47.000	31.000	43.000		
Mean	92.000	24.800	11.100	19.500		
±SD	30.030	17.606	10.908	15.248		
±SE	9.496	5.567	3.449	4.822		

Table 4: Multiple pairwise comparisons of colony forming unit (CFU) for *Candida albican* exposed to plasma using Tukey HSD

(I) time	(J) time	Mean Difference (I-J)	p value
Baseline	3 mins.	67.200	0.004
	6 mins.	80.900	0.001
	9 mins.	72.500	0.001
2	6 mins.	13.700	0.051
	9 mins.	5.300	1.000
3	9 mins.	-8.400	0.742

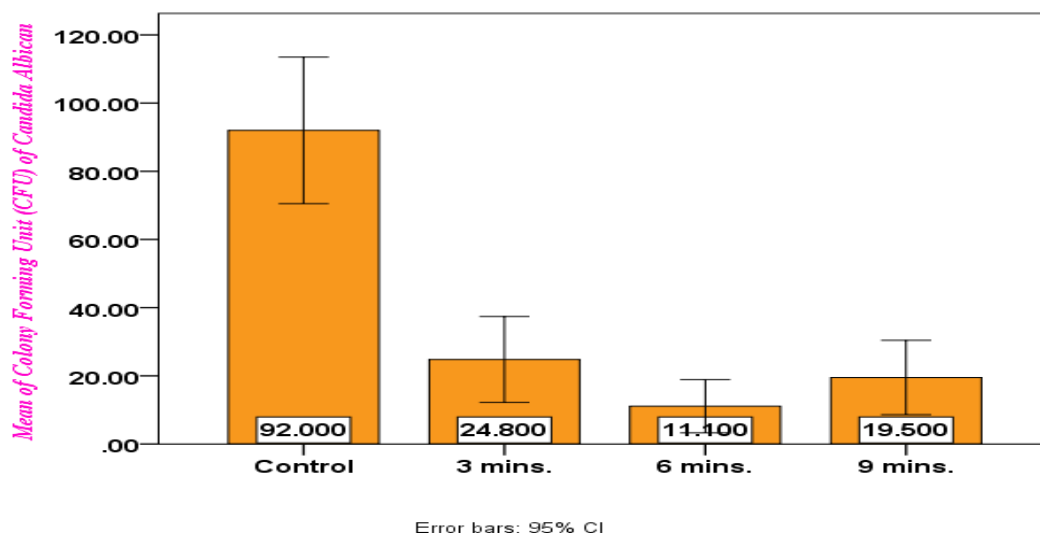


Figure 4: Sensitivities of *Candida albican* exposed to plasma at different exposure times (A) control (B) after 3 minutes (C) after 6 minutes (D) after 9 minutes.

Discussion

The reduction in the mean value of the bacterial number (CFU/ml) for *Streptococcus mutans* after treatment with plasma (study groups) was observed when compared with mean value before plasma exposure (control group). A reduction in viable count of bacterial number with a statistically highly significant difference after 3 and 6 minutes and statistically significant difference after 9 minutes when compared with control and an increase in the percentage of bacterial killing was observed with increasing exposure times until 6 minutes then after that there is increase in viable count of bacteria after 9 minutes. A statistically significant and highly significant differences were shown in the bacterial number (CFU/ml) when compared between each group (treatment group). The reduction in the mean value of the *C. albicans* (CFU/ml) after treatment with plasma (study groups) was observed when compared with mean value before plasma (control group). A reduction in viable count of *Candida* number with a statistically highly significant difference at all times when compared with control and an increase in the percentage of

Candida killing was observed with increasing exposure times until 6 minutes then after that there is increase in viable count of *Candida* after 9 minutes. No significant differences were shown in the *Candida* number (CFU/ml) when compared between each group. The antimicrobial effects are depend on the production of reactive oxygen (ROS) and nitrogen species (RNS) including charged particles, free radicals, electric fields, and electric radiation such as Ultraviolet radiation. These action guide to antimicrobial activity because of oxidation of DNA and cell membranes. Different parts of the pathogens are attacked by RNS and ROS, the cell wall is etched, and the cell membrane is harm by lipid peroxidation and disruption. The microbial RNA and DNA are weakened by strand breaks, base modification, and oxidative damage. In addition macromolecules, for example proteins may turn into unfolded or altered^(17, 20).

The current study agreed with other studies confirmed antimicrobial activity of CAP^(28,29). it disagreed with other study showed argon plasma irradiation effect had no

significant decrease of CFU for *S. mutans* between the control and treatment group⁽²⁷⁾. A time-dependent rise of the antimicrobial activity was noticed in this study, except when exposure to cold atmospheric plasma for 9 min, there is decrease in the antimicrobial effect. This may be because microorganism develop resistant to plasma after 9 minutes.

The susceptibilities of the two tested pathogens to CAP irradiation differ in this study. *S. mutans* showed some resistance to plasma-jet exposure. *Streptococci mutans* is a Gram-positive, non-motile -facultative anaerobe and smaller in comparison with the *Candida*. Its resistance to CAP jet irradiation may be caused by its small size. Another reason may be the construction of the cell wall of *Streptococci mutans*, that is comprised of strongly cross-linked murein⁽³⁰⁾.

Conclusion

Cold Atmospheric plasma (argon gas) jet have anti-microbial efficacy against *Streptococci mutans* and *Candida albicans*. but its effect on *Candida* more than on *Streptococci mutans*

Funding

This research received no external funding.

Data Availability Statement

Data are available from the authors upon reasonable request.

Conflict of interest

The authors reported that they have no conflicts of interest.

Acknowledgments

The authors would like to thank Mustansiriyah University (www.uomustansiriyah.edu.iq), Baghdad, Iraq, for their support in the present work.

References

1. Struzycka I. (2014) The oral microbiome in dental caries. *Pol J Microbiol*; 63(2):127-35. PMID: 25115106. <https://doi.org/10.33073/pjm-2014-018>
2. Lemos JA, Palmer SR, Zeng L, Wen ZT, Kajfasz JK, Freires IA, Abranches J, Brady LJ. (2019) The Biology of *Streptococcus mutans*. *Microbiol Spectr* ;7(1):10.1128. doi: 10.1128/microbiolspec. GPP3-0051-2018. <https://doi.org/10.1128/microbiolspec>
3. María Alejandra B, Mariano Daniel O. (2020) Virulence Factors of *Streptococcus mutans* Related to Dental Caries. *Staphylococcus and Streptococcus*. IntechOpen. DOI: <https://doi.org/10.5772/intechopen.85807>
4. Journal, Baghdad. (2009) The influence of He-Ne Laser (632.8 nm) on *Candida albicans* isolated from complete upper dentures: In vitro study. *Baghdad Science Journal*; 6(4): 790-796. DOI: <https://doi.org/10.21123/bsj.6.4.790-796>
5. Journal, Baghdad. (2015) The Inhibitory Effect of *Lactobacillus acidophilus* and *Lactobacillus plantarum* against *Candida albicans* Associated with Denture Stomatitis. *Baghdad Science Journal*; 12: 479-484. DOI: <https://doi.org/10.21123/bsj.12.3.479-484>
6. Christina Tsui, Eric F. Kong, Mary Ann Jabra-Rizk. (2016) Pathogenesis of *Candida albicans* biofilm, *Pathogens and Disease*, 74(4): ftw018. doi: <https://doi.org/10.1093/femspd/ftw018>
7. Vila T, Sultan AS, Montelongo-Jauregui D, Jabra-Rizk MA. (2020) Oral Candidiasis. A Disease of Opportunity. *J Fungi (Basel)*; 6(1):15. Doi: <https://doi.org/10.3390/jof6010015>
8. O'Donnell LE, Millhouse E, Sherry L, Kean R, Malcolm J, Nile CJ, Ramage G. (2015)

Polymicrobial Candida biofilms: friends and foe in the oral cavity. *FEMS Yeast Res*; 15(7):fov077. Doi:

<https://doi.org/10.1093/femsyr/fov077>

9. Allison DL, Willems H, Jayatilake J, Bruno VM, Peters BM, Shirtliff ME. (2016) Candida-Bacteria Interactions: Their Impact on Human Disease. *Microbiol Spectr*; 4(3). DOI: <https://doi.org/10.1128/microbiolspec.VMBF-0030-2016>

10. Ibrahim GA, Al Obaidi WA. (2013) Effect of small cardamom extracts on Mutans streptococci and Candida albicans in comparison to chlorhexidine gluconate and de-ionized water (In vivo study). *J Bagh Coll Dent*; 25(4):104-108. DOI:

<https://doi.org/10.12816/0015075>

11. Xiao J, Huang X, Alkhers N, Alzamil H, Alzoubi S, Wu TT, Castillo DA, Campbell F, Davis J, Herzog K, Billings R, Kopycka-Kedzierawski DT, Hajishengallis E, Koo H. (2018) Candida albicans and Early Childhood Caries: A Systematic Review and Meta-Analysis. *Caries Res*; 52 (1-2):102-112. Doi: <https://doi.org/10.1159/000481833>

12. Menon LU, Scoffield JA, Jackson JG and Zhang P (2022) Candida albicans and Early Childhood Caries. *Front. Dent. Med*; 3:849274. <https://doi.org/10.3389/fdmed.2022.849274>

13. Martin M. (2009) From distant stars to dental chairs- Plasmas May Promise Pain-free and durable Restorations. *AGD Impact* 37: 46.

14. Kong MG, Kroesen G, Morfill G, Nosenko T, Shimizu T, et al. (2009) Plasma medicine: an introductory review. *New J Phys* 11: 115012. DOI : <https://doi.org/10.1088/1367-2630/11/11/115012>

15. Hoffmann C, Berganza C, Zhang J (2013) Cold Atmospheric Plasma: methods of

production and application in dentistry and oncology. *Med Gas Res* 3: 21. Doi: <https://doi.org/10.1186/2045-9912-3-21>

16. Kieft, I. E., van Berkel, J. J. B. N., Kieft, E. R. & Stoffels, E. (2005) Radicals of plasma needle detected with fluorescent probe. In *Plasma Processes and Polymers*, chapter 22, pp. 295-308. Edited by R. d'Agostino, P. Favia, C. Oehr & M. R. Wertheimer. Berlin: Wiley-VCH. Kim, S. M. & Kim, J. I. (2006). Decomposition of biological macromolecules by plasma generated with helium and oxygen. *J Microbiol* 44: 466-47. <https://doi.org/10.1002/3527605584.ch22>

17. Lackmann J, Bandow J.E. (2014) Inactivation of microbes and macromolecules by atmospheric-pressure plasma jets. *Appl Microbiol Biotechnol*; 98: 6205-6213. doi: <https://doi.org/10.1007/s00253-014-5781-9>

18. Ranjan, R.; Krishnamraju, P.V.; Shankar, T.; Gowd, S. (2017) Nonthermal Plasma in Dentistry: An Update. *J. Int. Soc. Prev. Community Dent*; 7: 71-75. doi: https://doi.org/10.4103/jispcd.JISPCD_29_17

19. Masood SH, Mahamed SA. (2020) Effect of plasma treatment on some surface properties of acrylic resin polymer. *J Bagh Coll Dent*; 32(2): 22-5. DOI: <https://doi.org/10.26477/jbcd.v32i2.2890>

20. Jungbauer G, Moser D, Müller S, Pfister W, Sculean A, Eick S. (2021) The Antimicrobial Effect of Cold Atmospheric Plasma against Dental Pathogens-A Systematic Review of In-Vitro Studies. *Antibiotics*; 10 (2): 211. DOI: <https://doi.org/10.3390/antibiotics10020211>

21. Anber LM, Hamad TI. (2021) Effect of plasma treatment on the bond of soft denture liner to conventional and high impact acrylic

denture materials. *J Bagh Coll Dent*; 33(3):9-11. DOI: <https://doi.org/10.26477/jbcd.v33i3.2948>

22. Goree J, Liu B, Drake D, Stoffels E. (2007) Killing of *S. mutans* Bacteria Using a Plasma Needle at Atmospheric Pressure. *IEEE Trans Plasma Sci* 34: 1317- 1324. DOI: <https://doi.org/10.1109/PPPS.2007.4345643>

23. Yang B, Chen J, Yu Q, Li H, Lin M, et al. (2011) Oral bacterial deactivation using a low-temperature atmospheric argon plasma brush. *J Dent*; 9: 48-56. doi: <https://doi.org/10.1016/j.jdent.2010.10.002>

24. Borges A, Castaldelli N, Kostov K, de Morais Gouvêa Lima G, Lacerda Gontijo A, de Carvalho J, Yzumi Honda R, Yumi Koga-Ito C. (2017) Cold atmospheric pressure plasma jet modulates *Candida albicans* virulence traits. *Clin. Plasma Med*; 7: 9-15. <https://doi.org/10.1016/j.cpme.2017.06.002>

25. Sladek REJ, Stoffels E, Walraven R, Tiebeek PJA, Koolhoven RA (2004) Plasma treatment of dental cavities: a feasibility study. *IEEE Trans Plasma Sci* 32: 1540- 1543. <https://doi.org/10.1109/TPS.2004.832636>

26. Cain D, Hanks H, Weis M, Bottoms C, Lawson J. (2013) *Microbiology Laboratory Manual*. Collin County Community College District, McKinney, TX.

27. Abonti TR, Kaku M, Kojima S, Sumi H, Kojima S, Yamamoto T, Yashima Y, Miyahara H, Okino A, Kawata T, Tanne K, Tanimoto K. (2016) Irradiation effects of low temperature multi gas plasma jet on oral bacteria. *Dent Mater J*; 35(5):822-828. Doi: <https://doi.org/10.4012/dmj.2016-062>

28. Langner I, Kramer A, Matthes R, Rebert F, Kohler C, Koban I, Hübner N, Kohlmann T, Patrzyk M. (2019) Inhibition of microbial growth by cold atmospheric plasma compared with the antiseptics chlorhexidine digluconate, octenidine dihydrochloride, and polyhexanide. *Plasma Process Polym*: e1800162. <https://doi.org/10.1002/ppap.201800162>

29. Nima G, Harth-Chu E, Hiers RD, et al. (2021) Antibacterial efficacy of non-thermal atmospheric plasma against *Streptococcus mutans* biofilm grown on the surfaces of restorative resin composites. *Scientific Reports*; 11(1):23800. DOI: <https://doi.org/10.1038/s41598-021-03192-0>

30. Rupf S, Lehmann A, Hannig M, Schäfer B, Schubert A, Feldmann U, Schindler A. (2010) Killing of adherent oral microbes by a non-thermal atmospheric plasma jet. *J Med Microbiol*; 59(Pt2): 206-212. Doi: <https://doi.org/10.1099/jmm.0.013714-0>